

Simultaneous determination of erythromycin A in giant prawn and tilapia in Mekong region by stripping square wave voltammetry

*Minh, N. P., Lam, T. B. and Giao, N. T.

Department of Food Technology, Ho Chi Minh City University of Technology,
268 Ly Thuong Kiet Street, District 10, Ho Chi Minh City, Vietnam

Abstract: Erythromycin A (EA) is now one of antibiotics limited in seafood products in general and in giant freshwater prawns (*Macrobrachium rosenbergii*) and tilapia (*Oreochromis niloticus*) in particular while exporting to the US, EU, Japan, Canada. There are many methods used for analyzing this antibiotic in these aquatic species (e.g., ELISA, HPLC, LC-MS/MS, GC-MS). A new, sensitive, analytical approach for determination of erythromycin A using stripping square wave voltammetry at the slowly dropping mercury electrode was developed and validated to quantify this antibiotic with simple and short time analysis; the method is inexpensive and performs best at moderate concentrations of erythromycin A. Electrochemical signals were measured at potential wave -1430 mV. The optimal experimental parameters for the method were: supporting electrolyte ammonium acetate 0.1 M, pH 8.0, the solvents for dissolving erythromycin standard: acetonitril, $V_{\text{start}} = -400 \text{ mV}$, $V_{\text{stop}} = -1700 \text{ mV}$, $V_{\text{step}} = 6 \text{ mV}$, $V_{\text{pulse}} = 40 \text{ mV}$, $T_{\text{drop}} = 5000 \text{ ms}$, $V_{\text{electrolyse}} = -1100 \text{ mV}$, $T_{\text{electrolyse}} = 5 \text{ s}$. The method showed high recovery ($85.07 \div 96.50\%$), high sensitivity (lower limit of detection, $\text{LoD} = 0.57 \mu\text{g} \cdot \text{kg}^{-1}$ in giant prawn and $\text{LoD} = 0.52 \mu\text{g} \cdot \text{kg}^{-1}$ in tilapia) and high precision ($\text{RSD} 0.91 \div 2.1\%$) as well as excellent linearity ($r^2_{\text{adjusted}} \geq 0.99999$).

Keywords: Erythromycin A, giant freshwater prawn, tilapia, stripping square wave voltammetry, dropping mercury electrode

Introduction

Giant freshwater prawn (*Macrobrachium rosenbergii*) and Nile tilapia (*Oreochromis niloticus*) have been considered two of the most important species of freshwater aquaculture in Viet Nam, especially in the Mekong River Delta. Bacterial necrosis is a common disease observed in adult prawns. Bacterial necrosis has variously been termed as ‘black spot’, ‘brown spot’, ‘shell disease’ or chitinolytic bacterial disease. It is caused by the invasion of chitinolytic bacteria, which break down the chitin of the exoskeleton. *Aeromonas hydrophila*, *A. caviae*, *A. sorbia* and *Aeromonas* sp. All have been isolated from necrosis prawns. *Pseudomonas fluorescens*, *Aeromonas* sp., *Lactococcus garvieae* and *Edwardsiella tarda* were bacteria flora isolated from adult prawns. Meanwhile, the most significant diseases in Nile tilapia (*Oreochromis niloticus*) culture are caused by *Streptococcus iniae*, *Aeromonas hydrophila*, *Trichodina* sp., *Flexibacter* and *Edwardsiella* spp.

Erythromycins are broad spectrum antibiotics that exhibit high activity against nearly all Gram-positive and Gram-negative bacteria. Erythromycin A consists of a polyhydroxylactone and two sugars (Figure 1). Erythromycin is the antibiotic of choice against *Aeromonas hydrophila*, *A. caviae*, *A. sorbia*, *Aeromonas* sp. and *Pseudomonas fluorescens* [1, 2, 4, 16, 19, 22, 23].

According to Codex regulation (e.g., WHO/FAO, EU, US, Canada, Australia), erythromycin residue in seafood muscle must be lower than $100 \mu\text{g}/\text{kg}$. Viet Nameese Ministry of Agriculture and Rural Development regulates erythromycin as a limited antibiotic with maximum residual limit $200 \mu\text{g}/\text{kg}$. Methods for erythromycin analysis have evolved rapidly in the last 15 years (Table 1).

The aim of this work was to develop a fast scanning square wave voltammetry using a dropping mercury electrode to quantify erythromycin A. The results demonstrated that it could be used as a simple and rapid analytical screening technique for the detection of erythromycin in giant freshwater prawn and tilapia muscle.

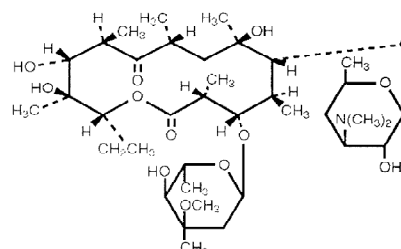


Figure 1. Chemical structure of erythromycin A

Materials and Methods

Reagents

The high purity antibiotic standards of erythromycin A, chloramphenicol, furazolidone, florfenicol, ciprofloxacin, colistin, and malachite

*Corresponding author.

Email: httk1983@gmail.com

Table 1. Some published papers on the methods of quantifying Erythromycin A from different samples

Year	Author	Sample	Method	LoD ($\mu\text{g}/\text{kg}$)
1994	Zierels G [26]	Egg, muscle, milk, liver, kidney of swan	HPLC	<10
1998	Yong-Xi Li [25]	Human plasma	LC-MS/MS	0.5*
1999	Kondo, T [15]	Human plasma	LC-MS/MS	0.05*
2000	Dreassi E [7]	Plasma: beef, pork, poultry	HPLC-UV	250
		Milk	HPLC-UV	25*
		Kidney, liver, muscle, gan, fat of beef, pork, poultry.	HPLC-UV	125*
2000	Huasheng Wang [12]	Drug, urine.	ASV-PGCE	5
LC-FL	Carmen Leal [3]	Chicken		400
ELISA	R. Draisci [8]	Beef		0.4
		Muscle and liver of beef	LC-MS/MS	50*
		Kidney of beef	LC-MS/MS	80*
2003	Stanley M. Billedeau [20]	Salmon	LC-ESI/MS	5, 16*
2003	Horie Masakazu [10]	Meat and seafood	LC-ESI-MS	10
2003	Michael P. Sche [17]	Manure	HPLC-MS/MS	0.4-11
2005	W. Xiao [24]	Drugs (propionate, base)	HPLC-ESI-MS	1
2006	A. Deuber [5]	Muscle	LC-MS/MS	0.25
2006	Hui Yun - Hua [13]	Tilapia	HPLC	400
2006	Jian Wang [14]	Fresh milk	LC-ESI/MS/MS	0.07
2006	Jiang HP [21]	Meat	LC-MS/MS	0.1
2007	Deng B [6]	Rat plasma	ECL	0.35
2008	Berrada Houda [11]	Meat and seafood	LC-ESI/MS	0.5
2008	Granja K [9]	Honey	LC-MS/MS	1.27, 5.0*
2009	P. Norouzi [18]	Human plasma, urine.	CV	2.4, 7.0*

* LoQ

green were purchased from Vietnam Central Institute of Pharmacy. Methanol and acetonitrile (HPLC grade) were obtained from J. T. Baker. All reagents were analytic grade and all solutions were prepared by dissolving appropriate weights in bi-distilled water.

Apparatus

A fast scanning, stripping, square wave voltammetry at the slowly dropping mercury electrode was performed in the ANALYZER SQF-505. The mercury dropping electrode was used as a working electrode, silver/silver chloride (saturated KCl) as a reference electrode, and a platinum wire as an auxiliary one.

Sample extraction and clean-up procedure

Primary extraction

A 5 g aliquot of a blank or spiked minced muscle sample was mixed with a small volume of erythromycin standard. After a 15 min equilibration period, the tissues were mixed vigorously for 15 min with 25 ml Tris buffer (0.1M; pH 10.5). After a 10 min centrifugation at 3000 g and 4°C, the supernatant was transferred to a polypropylene tube and the solid residue extracted a second time with 25 ml Tris buffer. Acetic acid (600 μl) and 5 ml sodium tungstate buffer (0.15M) were added to precipitate the proteins. After equilibration for one hour at 4°C, the samples were centrifuged at 3000 g for 10 min. The supernatants were further filtered through a plug of glass wool.

Solid phase extraction

The 6-cm³ HLB OASIS extraction cartridges (200 mg) were prepared and conditioned with 10 ml methanol and 10 ml water. The biological samples were placed at the top of the column. Two wash solution volumes were applied before erythromycin elution: 20 ml methanol-water (5:95, v/v) and 5 ml hexane. After the last washing step, the OASIS columns were vacuum-dried for 10 min. Erythromycin

was finally eluted with 5 ml methanol-ammonia 30% (95:5, v/v) and evaporated dry under a nitrogen flow. The extracts were dissolved in 500 μl NH₄AC-ACN (80/20 v/v), transferred to Eppendorf tubes and centrifuged at 3000 g for 10 min. Aliquots of the supernatant were transferred into the voltammetric cell with 2,500 mL of ammonium acetate 0.1 M, pH 8.0 before being quantified by Analyzer SQF-505 in mode stripping, square wave, voltammetry.

Results and Discussion

Voltammetric behavior of erythromycin at the slowly dropping electrode

Effect of supporting electrolytes and pH values on the adsorptive peak current of erythromycin has been strongly affected by the type of supporting electrolyte. To study the adsorptive behavior of erythromycin, different supporting electrolytes including sodium acetate, ammonium acetate, citrate-phosphate, borax, and Tris buffers were examined. Ammonium acetate buffer is recommended to complete these studies because erythromycin showed the highest peak current and the best peak shape (Table 2).

The effect of pH of ammonium acetate buffer on the peak current was examined from 7.0 to 10.0. Erythromycin showed highest peak current at pH 8.0 ($E_{1/2} = -1438$ mV, $I = 351.7 \pm 5.7$ nA). Hence ammonium acetate buffer (pH 8.0) was selected for further investigations

The effect of the ionic strength of supporting electrolyte was examined at pH 8.0 over the range from 0.05-0.25 M. Erythromycin showed highest peak current at ammonium acetate 0.1M ($E_{1/2} = -1438$ mV, $I = 254.8 \pm 10.2$ nA). So this value was selected for further studies (Table 3).

Effect of the solvents for dissolving erythromycin A standard on the peak current were examined. Among methanol, acetonitril, and ethyl acetate, the peak current increased with a maximum at acetonitril ($E_{1/2} = -1438$ mV, $I = 189.2 \pm 3.5$ nA). So acetonitril was selected for subsequent work (Table 4).

Table 2. Peak current of erythromycin A was affected by supporting electrolytes, pH values

pH	5.0		6.0		7.0		8.0		9.0		10.0	
Supporting electrolytes	Mean ± SD	RSD (%)	Mean ± SD	RSD (%)	Mean ± SD	RSD (%)	Mean ± SD	RSD (%)	Mean ± SD	RSD (%)	Mean ± SD	RSD (%)
Natri acetate	56.67 ^b ± 1.1	1.9	35.5 ^a ± 2.3	6.6	255.5 ^d ± 7.3	2.8	333.4 ^e ± 4.7	1.4	236.2 ^c ± 7.7	3.3	254 ^d ± 4.7	1.9
Ammonium acetate					210.3 ^a ± 5.4	2.6	351.7^d ± 5.7	1.6	216.5 ^b ± 2.7	1.2	263.1 ^c ± 1.6	0.6
Citrat-phosphate			207.7 ^d ± 6.0	2.9	168.2 ^a ± 2.3	1.4	194.4 ^b ± 2.6	1.4	229.4 ^e ± 2.1	0.9	200.9 ^c ± 2.0	1.0
Tris					180.0 ^d ± 13.1	7.3	27.5 ^a ± 0.3	1.1	53.4 ^b ± 3.6	6.7	126.4 ^c ± 9.7	7.7
Borax							168.1 ^a ± 1.6	0.9	255.5 ^c ± 6.5	2.6	173.9 ^b ± 1.8	1.0

* Each value was the mean of 5 samples (n = 5).

Table 3. Erythromycin A peak current was affected by ionic strength of ammonium acetate

Ionic strength (M)	0.05		0.1		0.15		0.2		0.25	
	Mean ± SD	RSD (%)	Mean ± SD	RSD (%)	Mean ± SD	RSD (%)	Mean ± SD	RSD (%)	Mean ± SD	RSD (%)
	210 ^a ± 7.1	3.4	254.8^d ± 10.2	4.0	213.7 ^c ± 10.1	4.7	192.1 ^b ± 2.2	1.1	173.2 ^a ± 1.8	1.0

* Each value was the mean of 5 samples (n = 5).

Table 4. Peak current of erythromycin A was affected by solvents

Ethyl acetate		Acetonitril		Methanol	
Mean ± SD	RSD (%)	Mean ± SD	RSD (%)	Mean ± SD	RSD (%)
183.6 ^b ± 1.5	0.8	189.2^c ± 3.5	1.9	166.3 ^a ± 5.5	3.3

* Each value was the mean of 5 samples (n = 5).

Table 5. Peak current of erythromycin A was affected by V_{start}

V _{start} (mV)	-400	-500	-600	-700	-800	-900	-1000	-1100
Mean ± SD	106.5^g ± 4.7	97 ^f ± 3.4	79.5 ^e ± 0.8	71.5 ^d ± 4.3	93.3 ^f ± 4.0	45.0 ^e ± 2.6	23.4 ^b ± 1.0	14.8 ^a ± 0.9
RSD (%)	4.4	3.5	1.0	6.0	4.3	5.8	4.3	6.2

* Each value was the mean of 5 samples (n = 5).

Optimization of measurement conditions

Effect of forward scanning (0 to -1800 mV) and reverse scanning (-1800mV to 0) on the peak current signal was examined. The forward scanning (0 to -1800 mV) showed high peak. Meanwhile, the peak current of the reverse scanning (-1800mV to 0) was too low. So the forward scanning (0 to -1800 mV) was chosen for further investigations.

Effect of V_{start}. Mode PSA-F, forward scanning, V_{stop}: -1800 mV, V_{step}: 4 mV, V_{pulse}: 30 mV, T_{drop}: 3000 ms, V_{electrolise}: -700 mV, T_{electrolise}: 6 s, T_{stabilize}: 1 s. Examining V_{start} from -400 mV to -1100 mV. V_{start} was optimum at -400 mV (E_{1/2} = -1430 mV, I = 106.5 ± 4.7 nA) (Table 5).

Effect of V_{stop}. Mode PSA-F, forward scanning, V_{start}: -400 mV, V_{step}: 4 mV, V_{pulse}: 30 mV, T_{drop}: 3000 ms, V_{electrolise}: -700 mV, T_{electrolise}: 6 s, T_{stabilize}: 1 s. Examining V_{stop} from -1700 mV to -2000 mV. V_{start} was optimum at -1700 mV (E_{1/2} = -1430 mV, I = 136.7 ± 3.9 nA) (Table 6).

Effect of V_{step}. Mode PSA-F, forward scanning, V_{start}: -400 mV, V_{stop}: -1700 mV, V_{pulse}: 30 mV, T_{drop}: 3000 ms, V_{electrolise}: -700 mV, T_{electrolise}: 6 s, T_{stabilize}: 1 s. Examining V_{step} from 4 mV to 10 mV. V_{step} was

optimum at 6.0 mV (E_{1/2} = -1430 mV, I = 214.6 ± 13.1 nA) (Table 7).

Effect of V_{pulse}. Mode PSA-F, forward scanning, V_{start}: -400 mV, V_{stop}: -1700 mV, V_{step}: 6.0 mV, T_{drop}: 3000 ms, V_{electrolise}: -700 mV, T_{electrolise}: 6 s, T_{stabilize}: 1 s. Examining V_{pulse} from 10 mV to 40mV. V_{pulse} was optimum at 40 mV (E_{1/2} = -1430 mV, I = 692.6 ± 14.9 nA) (Table 8).

Effect of T_{drop}. Mode PSA-F, forward scanning, V_{start}: -400 mV, V_{stop}: -1700 mV, V_{step}: 6 mV, V_{pulse}: 40 mV, V_{electrolise}: -700 mV, T_{electrolise}: 6 s, T_{stabilize}: 1 s. Examining T_{drop} from 1000 ms to 5,000 ms. T_{drop} was optimum at 5,000 ms (E_{1/2} = -1430 mV, I = 381.3 ± 2.9 nA) (Table 9).

Effect of T_{electrolise}. Mode PSA-F, forward scanning, V_{start}: -400 mV, V_{stop}: -1700 mV, V_{step}: 6 mV, V_{pulse}: 40 mV, T_{drop}: 5,000 ms, V_{electrolise}: -700 mV, T_{stabilize}: 1 s. Examining T_{electrolise} from 3s to 6s. T_{electrolise} was optimum at 5 s (E_{1/2} = -1430 mV, I = 1717.0 ± 13.7 nA) (Table 10).

Effect of V_{electrolise}. Mode PSA-F, forward scanning, V_{start}: -400 mV, V_{stop}: -1700 mV, V_{step}: 6 mV, V_{pulse}: 40 mV, T_{drop}: 5,000 ms, T_{electrolise}: 5 s, T_{stabilize}: 1 s. Examining V_{electrolise} from -400 mV to -1400 mV.

Table 6. Peak current of erythromycin A was affected by V_{stop}

V_{stop} (mV)	-1500.0	-1600.0	-1700.0	-1800.0
Mean \pm SD	104 ^a \pm 1.0	118.2 ^b \pm 1.4	136.7 ^c \pm 3.9	120.1 ^b \pm 1.1
RSD (%)	0.9	1.2	2.9	0.9

^a Each value was the mean of 5 samples (n = 5).

Table 7. Peak current of erythromycin A was affected by V_{step}

V_{step} (mV)	4.0	6.0	8.0	10.0
Mean \pm SD	162.8 ^a \pm 5.8	214.6 ^c \pm 13.1	176.9 ^b \pm 8.3	165.0 ^{ab} \pm 10.9
RSD (%)	3.5	6.1	4.7	6.6

^a Each value was the mean of 5 samples (n = 5).

Table 8. Peak current of erythromycin A was affected by V_{pulse}

V_{pulse} (mV)	10	20	30	40
Mean \pm SD	230.6 ^a \pm 2.7	388.4 ^b \pm 12.7	528.0 ^c \pm 8.0	692.6 ^d \pm 14.9
RSD (%)	1.2	3.3	1.5	2.2

^a Each value was the mean of 5 samples (n = 5).

Table 9. Peak current of erythromycin A was affected by T_{drop}

T_{drop} (ms)	1,000	2,000	3,000	4,000	5,000
Mean \pm SD	128.3 ^a \pm 1.2	197.9 ^b \pm 1.9	269.1 ^c \pm 12.9	323.2 ^d \pm 3.3	381.3 ^e \pm 2.9
RSD (%)	0.9	1.0	4.8	1.0	0.8

^a Each value was the mean of 5 samples (n = 5).

Table 10. Peak current of erythromycin A was affected by $T_{electrolise}$

$T_{electrolise}$ (s)	3	4	5	6
Mean \pm SD	1353.6 ^a \pm 10.8	1555.4 ^b \pm 13.0	1717.0 ^d \pm 13.7	1655.4 ^c \pm 5.0
RSD (%)	0.8	0.8	0.8	0.3

^a Each value was the mean of 5 samples (n = 5).

Table 11. Peak current of erythromycin A was affected by $V_{electrolise}$

$V_{electrolise}$ (mV)	-400.0	-900.0	-1100.0	-1400.0
Mean \pm SD	1709.0 ^b \pm 17.3	1815.0 ^c \pm 3.7	1863.2 ^c \pm 24.1	1593.4 ^a \pm 13.5
RSD (%)	1.0	0.2	1.3	0.8

^a Each value was the mean of 5 samples (n = 5).

$V_{electrolise}$ was optimum at -1100 mV ($E_{1/2} = -1438$ mV, $I = 1863.2 \pm 24.1$ nA) (Table 11).

Calibration

For the calibration curves and detection limit, a 25 mL supporting electrolyte ammonium acetate 0.1M, pH 8.0 was transferred to the cell and spiked with 5 μ L, 10 μ L, 20 μ L, 30 μ L, 40 μ L, 50 μ L, 60 μ L, 70 μ L, 80 μ L, 90 μ L of stock 250 ppm solution of erythromycin in pure acetonitril. The concentrations of erythromycin in the cell were 50 μ g/kg, 100 μ g/kg, 200 μ g/kg, 300 μ g/kg, 400 μ g/kg, 500 μ g/kg, 600 μ g/kg, 700 μ g/kg, 800 μ g/kg, 900 μ g/kg respectively. Mode PSA-F, V_{start} : -400 mV, V_{stop} : -1700 mV, V_{step} : 6 mV, V_{pulse} : 40 mV, T_{drop} : 5000 ms, $T_{electrolise}$: 5 s, $V_{electrolise}$: -1100 mV, $T_{stabilize}$: 1 s.

A detection limit of 0.57 μ g/kg was obtained for erythromycin. A linear behavior was also observed with a correlation coefficient $r^2_{adjust} = 1.0$ (Figure 2).

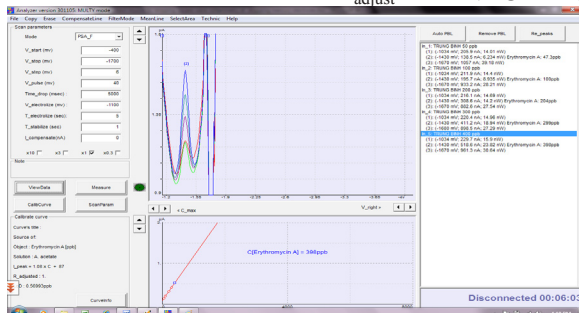


Figure 2. Calibration curve of erythromycin A

Interference

Effect of Interferences on the effect of co-existing ions was examined by introducing different concentrations of selected ions to the voltametric cell and recording the corresponding voltammogram using the conditions selected above. It was observed that the additions of 0-5 ppm K^+ , Na^+ , Ca^{2+} , Mg^{2+} , Fe^{3+} , Cl^- , SO_4^{2-} , HPO_4^{2-} ions had no effect ($< \pm 5\%$) on the peak response.

Sample analysis

In giant freshwater prawn samples, the recovery rate were: 90.40 \div 96.50 %, $LoD: 0.80 \mu\text{g.kg}^{-1}$, $R^2_{adjust}: 0.99999$, $RSD: 0.91 \div 1.58$ %. (Figure 3). In tilapia samples the recovery rate were: 85.07 \div 88.56%, $MDL: 0.52 \mu\text{g.kg}^{-1}$, $R_{adjust}: 1.0$, $RSD: 0.80 \div 2.10$ %. (Fig. 4)

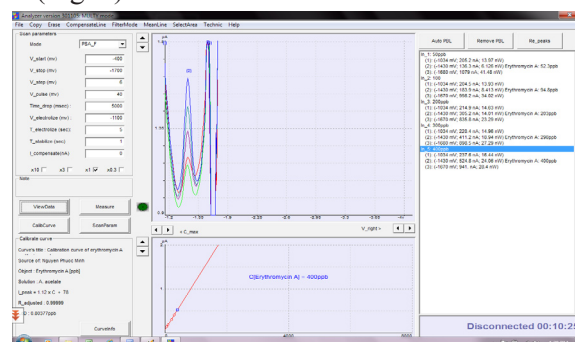


Figure 3. Calibration curve of erythromycin A in giant prawn muscle

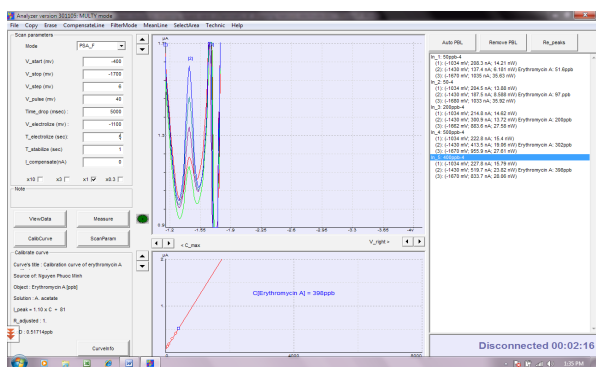


Figure 4. Calibration curve of erythromycin A in tilapia sample

For the comparison results between SWV and LC-MS/MS method, dosed giant prawn and tilapia samples were obtained through medication at 100 mg erythromycin·kg⁻¹ prawn body weight⁻¹·d⁻¹ for 7 days; sampled at 7, 8, and 9 days post-dosing. These dosed samples (high, medium, low) were divided in two groups: samples in group A were analyzed by Square Wave Voltammetry, samples in group B were controlled by LC-MS/MS via Intertek Vietnam Ltd. Close homogeneity could be seen between the two analyzing methods (Table 12, 13).

Validation of quantification method

Linearity

The linearity was evaluated by least squares, linear regression. The calibration curves constructed for erythromycin were linear over the concentration range of 50 ÷ 400 µg/kg. Peak areas of erythromycin were plotted versus its concentration and linear regression analysis performed on the resultant curve. A correlation coefficient of $R^2_{\text{adjust}} = 1.0$ with %R.S.D. values ranging from 0.4 ÷ 3.7 % across the concentration range studied were obtained (Table 14). The regression equation for the calibration curve was $Y=1.08 \cdot X + 87$.

LOD

The LOD was the lowest amount of measured analyte that may be detected to produce a response which is significantly different from that of a blank. Limit of detection was obtained by calculations based on the standard deviation of the response (δ) (here the current) which is obtained from blank with 5 replicas and (S) is the slope of the calibration curve according to equation $LOD=3.3(\delta/S)$. The LOD for erythromycin was 0.57 µg/kg (Figure 2).

Precision, accuracy and recovery

Precision was investigated by the intra- and inter-day (n = 6) assays at three different concentrations with respect to both repeatability and reproducibility.

Repeatability was investigated by injecting six replicate samples of each of the 100, 200, 300 µg/kg standards. Inter-day precision was assessed by injecting the same three concentrations over 3 consecutive days. Accuracy (relative error, RE, %) was calculated by assessing the agreement between measured and nominal concentrations of the fortified samples. Recovery was assessed as erythromycin A concentrations of 100, 200, 300 µg/kg and the mean value was calculated (Table 15, 16; Figure 5, 6).

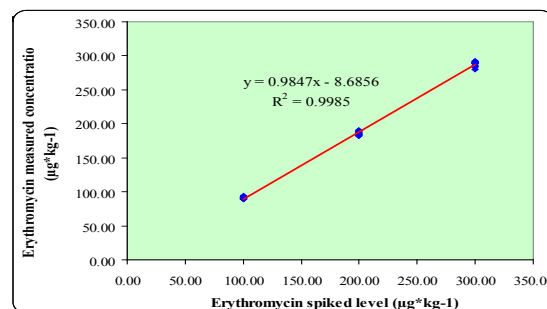


Figure 5. Erythromycin concentration was detected on prawn samples at different times and levels

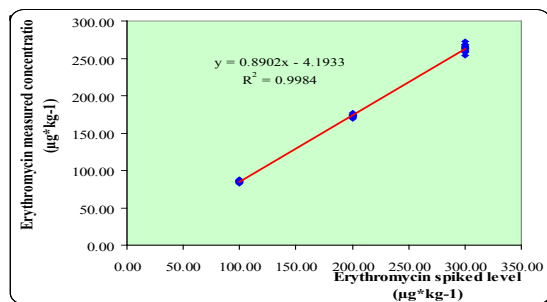


Figure 6. Erythromycin concentration was detected on fish samples at different times and levels

Differentiation

The differentiation of the method was checked by monitoring standard solutions of erythromycin A in the presence of other antibiotic components. The peak response ($E_{1/2}$) of erythromycin A ($E_{1/2} = -1430$ mV) was separated, independent and distinguished from ones obtained in chloramphenicol ($E_{1/2} = -196$ mV), furazolidone ($E_{1/2} = -1152$ mV), florfenicol ($E_{1/2} = -78$ mV), enrofloxacin, ciprofloxacin ($E_{1/2} = -1336$ mV), colistin ($E_{1/2} = -1120$ mV) malachite green ($E_{1/2} = -1228$ mV). Hence, the determination of erythromycin by SWV was considered having not only “screening” but also “confirming” abilities.

Application

Giant freshwater prawn and tilapia samples from ten provinces in the Mekong River Delta were analyzed to survey the erythromycin residue. Residual results are displayed figures 7 and 8.

Conclusion

A new analytical procedure based Square Wave

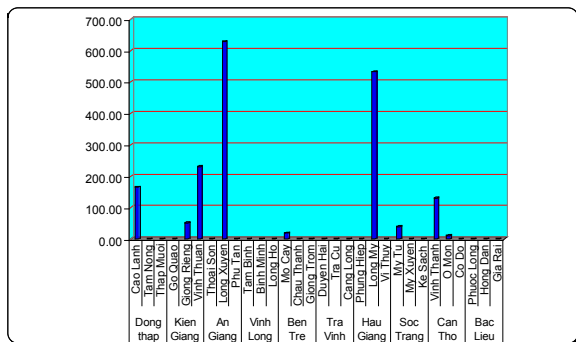


Figure 7. Erythromycin surveillance in prawn aquaculture at ten provinces, three districts in each province of Mekong Region, Vietnam

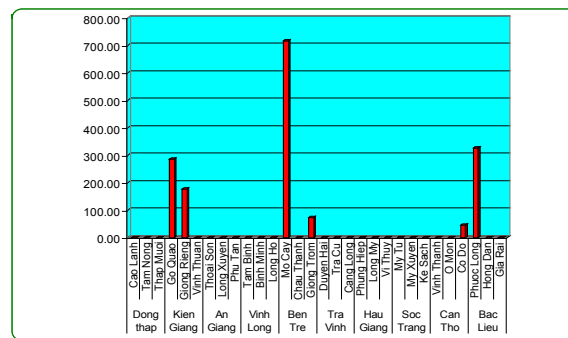


Figure 8. Erythromycin surveillance in tilapia aquaculture at ten provinces, three districts in each province of Mekong Region, Vietnam

Table 12. Comparison homogeneity of two analyzing methods in giant prawn muscle

Sample I.D	SWV (LOD = 0.8 µg*kg ⁻¹)			LC-MS/MS (LOD = 10 µg*kg ⁻¹)		
	Result (µg*kg ⁻¹)	Mean ± SD (µg*kg ⁻¹)	RSD (%)	Result (µg*kg ⁻¹)	Mean ± SD (µg*kg ⁻¹)	RSD (%)
CCP - Blank	N.D	N.A	N.A	N.D	N.A	N.A
CCP - Blank	N.D	N.A	N.A	N.D	N.A	N.A
CCP - III	51.37			50.73		
CCP - III	50.10	50.75 ^a ± 0.59	1.17	50.89	52.61 ^a ± 3.72	7.06
CCP - III	50.68			50.81		
CCP - III	65.45			75.82		
CCP - III	64.97	65.48 ^b ± 0.53	0.80	68.00	70.49 ^b ± 2.41	3.42
CCP - III	66.02			70.65		
CCP - III	80.61			74.60		
CCP - III	79.16	80.00 ^c ± 0.75	0.94	85.12	80.23 ^c ± 5.30	6.61
CCP - III	80.22			80.98		

*LOD: Limit of detection.
 **N.D: Not detected.
 ***N.A: Non application.
 ****Each value was the mean of 3 samples.

Table 13. Comparison homogeneity of two analyzing methods in tilapia muscle

Sample I.D	SWV (LOD = 0.52 µg*kg ⁻¹)			LC-MS/MS (LOD = 10 µg*kg ⁻¹)		
	Result (mg*kg ⁻¹)	Mean ± SD (mg*kg ⁻¹)	R.S.D (%)	Result (mg*kg ⁻¹)	Mean ± SD (mg*kg ⁻¹)	R.S.D (%)
TL - Blank	N.D	N.A	N.A	N.D	N.A	N.A
TL - Blank	N.D	N.A	N.A	N.D	N.A	N.A
TL - Blank	N.D	N.A	N.A	N.D	N.A	N.A
TL - I	1.31			1.23		
TL - I	1.27	1.29 ^a ± 0.02	1.61	1.28	1.26 ^a ± 0.03	2.10
TL - I	1.30			1.27		
TL - II	1.95			3.14		
TL - II	2.09	2.02 ^b ± 0.07	3.47	2.72	2.72 ^b ± 0.43	15.64
TL - II	2.02			2.29		
TL - II	2.80			2.80		
TL - II	2.80	2.78 ^c ± 0.03	1.25	2.80	2.80 ^b ± 0.01	0.21
TL - II	2.74			2.81		

*LOD: Limit of detection.
 **N.D: Not detected.
 ***N.A: Non application.
 ****Each value was the mean of 3 samples.

Table 14. Linear range in regression analysis of erythromycin

Erythromycin A concentration (ppb)	50.0	100.0	200.0	300.0	400.0
Peak current (Mean ± SD)	138.5 ^a ± 5.1	194.0 ^b ± 3.9	305.2 ^c ± 5.2	411.2 ^d ± 1.8	524.8 ^e ± 14.3
RSD (%)	3.7	2.0	1.6	0.4	2.7

* Each value was the mean of 5 samples.

Table 15. Precision (RSD %), accuracy (RE %) and recovery of erythromycin A in giant freshwater prawn muscles

Day	Spike level (µg*kg ⁻¹)	Measured concentration (mean ± SD, µg*kg ⁻¹)	RSD (%)	RE (%)
1	100	91.45 ^a ± 1.44	1.58	91.45
2	100	90.40 ^a ± 1.25	1.38	90.40
3	100	90.92 ^a ± 1.43	1.57	90.92
1	200	187.23 ^b ± 2.79	1.49	93.61
2	200	184.76 ^b ± 1.97	1.07	92.38
3	200	185.18 ^b ± 2.43	1.31	92.59
1	300	286.03 ^c ± 4.01	1.40	95.34
2	300	288.27 ^c ± 2.71	0.94	96.09
3	300	289.50 ^c ± 2.65	0.91	96.50

Table 16. Precision (RSD %), accuracy (RE %) and recovery of erythromycin A in tilapia muscles

Day	Spike level (µg*kg ⁻¹)	Measured concentration (mean ± SD, µg*kg ⁻¹)	RSD (%)	RE (%)
1	100	85.07 ^a ± 1.26	1.48	85.07
2	100	85.34 ^a ± 1.79	2.10	85.34
3	100	85.31 ^a ± 1.24	1.45	85.31
1	200	173.25 ^b ± 2.34	1.35	86.63
2	200	173.03 ^b ± 2.09	1.21	86.51
3	200	172.82 ^b ± 1.39	0.80	86.41
1	300	261.62 ^c ± 4.53	1.73	87.21
2	300	262.57 ^c ± 3.42	1.30	87.52
3	300	265.68 ^c ± 5.38	2.02	88.56

* Each value was the mean of 6 samples.

Table 17. Erythromycin residue of prawn samples from ten provinces, three districts in each province in the Mekong River Delta

No	Province	District	Giant Freshwater Prawn					Mean ($\mu\text{g}^*\text{kg}^{-1}$)	RSD (%)
			M1	M2	M3	M4	M5		
1	Dong Thap	Cao Lanh	169.00	164.00	171.00	159.00	162.00	165.00 ^f	3.00
		Tam Nong	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		Thap Muoi	N.D	N.D	N.D	N.D	N.D	N.D	N.D
2	Kien Giang	Go Quao	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		Giong Rieng	49.60	52.10	48.90	51.00	51.30	50.58 ^d	2.58
		Vinh Thuan	232.40	235.10	230.20	228.70	229.50	231.18 ^e	1.12
3	An Giang	Thoai Son	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		Long Xuyen	626.10	630.40	628.90	631.80	627.30	628.90 ⁱ	0.36
		Phu Tan	N.D	N.D	N.D	N.D	N.D	N.D	N.D
4	Vinh Long	Tam Binh	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		Binh Minh	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		Long Ho	N.D	N.D	N.D	N.D	N.D	N.D	N.D
5	Ben Tre	Mo Cay	18.00	18.70	19.20	17.90	18.60	18.48 ^b	2.90
		Chau Thanh	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		Giong Trom	N.D	N.D	N.D	N.D	N.D	N.D	N.D
6	Tra Vinh	Duyen Hai	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		Tra Cu	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		Cang Long	N.D	N.D	N.D	N.D	N.D	N.D	N.D
7	Hau Giang	Phung Hiep	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		Long My	531.70	529.50	533.10	528.90	541.00	532.84 ^h	0.91
		Vi Thuy	N.D	N.D	N.D	N.D	N.D	N.D	N.D
8	Soc Trang	My Tu	38.90	40.00	39.30	39.60	38.90	39.34 ^c	1.20
		My Xuyen	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		Ke Sach	N.D	N.D	N.D	N.D	N.D	N.D	N.D
9	Can Tho	Vinh Thanh	129.30	130.10	128.90	128.20	130.40	129.38 ^e	0.69
		O Mon	10.50	10.30	11.10	10.70	10.90	10.70 ^a	2.96
		Co Do	N.D	N.D	N.D	N.D	N.D	N.D	N.D
10	Bac Lieu	Phuoc Long	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		Hong Dan	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		Gia Rai	N.D	N.D	N.D	N.D	N.D	N.D	N.D

*N. D: Not dedected

Table 18. Erythromycin residue of tilapia samples from ten provinces, three districts in each province in the Mekong River Delta

No	Province	District	Tilapia					Mean ($\mu\text{g}^*\text{kg}^{-1}$)	RSD (%)
			M1	M2	M3	M4	M5		
1	Dong Thap	Cao Lanh	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		Tam Nong	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		Thap Muoi	N.D	N.D	N.D	N.D	N.D	N.D	N.D
2	Kien Giang	Go Quao	289.4	287.5	290.3	279.9	280.8	285.6 ^d	1.71
		Giong Rieng	175.2	177.9	176.3	175.9	177.8	176.6 ^c	0.67
		Vinh Thuan	N.D	N.D	N.D	N.D	N.D	N.D	N.D
3	An Giang	Thoai Son	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		Long Xuyen	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		Phu Tan	N.D	N.D	N.D	N.D	N.D	N.D	N.D
4	Vinh Long	Tam Binh	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		Binh Minh	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		Long Ho	N.D	N.D	N.D	N.D	N.D	N.D	N.D
5	Ben Tre	Mo Cay	713.0	719.2	720.0	715.8	716.9	716.9 ^f	0.39
		Chau Thanh	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		Giong Trom	72.5	73.1	72.8	74.0	72.7	73.0 ^b	0.81
6	Tra Vinh	Duyen Hai	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		Tra Cu	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		Cang Long	N.D	N.D	N.D	N.D	N.D	N.D	N.D
7	Hau Giang	Phung Hiep	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		Long My	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		Vi Thuy	N.D	N.D	N.D	N.D	N.D	N.D	N.D
8	Soc Trang	My Tu	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		My Xuyen	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		Ke Sach	N.D	N.D	N.D	N.D	N.D	N.D	N.D
9	Can Tho	Vinh Thanh	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		O Mon	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		Co Do	45.6	47.1	44.9	45.2	45.0	45.6 ^a	1.98
10	Bac Lieu	Phuoc Long	327.4	328.4	319.7	326.6	326.9	325.8 ^e	1.07
		Hong Dan	N.D	N.D	N.D	N.D	N.D	N.D	N.D
		Gia Rai	N.D	N.D	N.D	N.D	N.D	N.D	N.D

*N. D: Not dedected.

Voltammetry had been developed for simultaneous determination of erythromycin in giant prawn and tilapia. The proposed method was simple, quick, economical, and sensitive. It should be extensively used for veterinary drug residue screening in food surveillance programs.

Acknowledgements

I deeply thank Dr Tran Bich Lam – HCM University of Technology, Dr Nguyen Trong Giao – VietNam_Russia Tropical Center, South Branch in their technical assistance.

References

- Ahmed, H. Al-Harbi (2003). Bacterial flora of freshwater prawn, *Macrobrachium rosenbergii* (de Man), cultured in concrete tanks in Saudi Arabia. *Journal of Applied Aquaculture*, 14, 113 – 124.
- Be, L. M. (2002). Investigation on diseases of giant freshwater prawn (*Macrobrachium rosenbergii*) in ponds and rice-prawn farming systems in An Giang province. Msc. thesis (in Vietnamese).
- Billedeau, S.M., Heinze, T.M. and Siitonen, P.H. (2003). Liquid chromatography analysis of erythromycin A in salmon tissue by electrochemical detection with confirmation by electrospray ionization mass spectrometry. *Journal of Agriculture and Food Chemistry*, 51, 1534–1538.
- Berrada, H., Borrull, F., Font, G. and Marcé, R.M. (2008). Determination of macrolide antibiotics in meat and fish using pressurized liquid extraction and liquid chromatography–mass spectrometry. *Journal of Chromatography A*, 1208, 83-89.
- Chen, S.C., Lin, Y.D., Liaw, L.L. and Wang, P.C. (2001). *Lactococcus garvieae* infection in the giant freshwater prawn *Macrobrachium rosenbergii* confirmed by polymerase chain reaction and 16S rDNA sequencing. *Diseases of Aquatic Organisms*, 45, 45-52.
- Cheng, W. and Chen, J.C. (1998). Isolation and characterization of an Enterococcus like bacterium causing muscle necrosis and mortality in *Macrobrachium rosenbergii* in Taiwan. *Diseases of Aquatic Organisms*, 34, 93-101.
- Dat, N.T. (2002). Investigation on parasite and bacteria diseases in giant freshwater prawns (*Macrobrachium rosenbergii*) cultured in pond and rice-prawn with low density. Msc. Thesis (in Vietnamese).
- Deubel, A., Fandiño, A.S., Sörgel, F. and Holzgrabe, U. (2006). Determination of Erythromycin and related substances in commercial samples using liquid chromatography/ion trap mass spectrometry. *Journal of Chromatography A* 1136, 39-47.
- Deng, B., Kang, Y., Li, X. and Xu, Q. (2007). Determination of Erythromycin in rat plasma with capillary electrophoresis-electrochemiluminescence detection of tris (2, 2'-bipyridyl) ruthenium (II). *Journal of chromatography B*, 857, 136-141.
- Dreassi, E., Corti, P., Bezzini, F. and Furlanetto, S. (2000). High-performance liquid chromatographic assay of erythromycin from biological matrix using electrochemical or ultraviolet detection. *Analyst*, 125, 1077-1081.
- Draisci, R., Delli, Q.F., Achene, L., Volpe, G., Palleschi, L. and Palleschi, G. (2001). A new electrochemical enzyme-linked immunosorbent assay for the screening of macrolide antibiotic residues in bovine meat. *Analyst*, 126, 1942–1946.
- Granja, R., Nino, A.M., Zucchetti, R., Niño, R.M., Patel, R. and Salerno, A.G. (2009). Determination of erythromycin and tylosin residues in honey by LC-MS/MS. *JAOAC Int.*, 92, 975-980.
- Hui, Y.H., Yu, H.J., Cai, Y.X. and Zhou, P.G. (2006). Residual determination of erythromycin in tilapia by high performance liquid chromatography. *Marine Fisheries*, 28, 321-325.
- Kondo, T., Dote, N., Hagimoto, T. and Yoshimura, Y. (1999). Application of liquid chromatography-turbo ion spray tandem mass spectrometry for quantitative analysis of a potent motilin receptor agonist, EM574, and its metabolites in human plasma. *J Chromatogr B Biomed Sci Appl.*, 29, 734, 101-112.
- Lalitha, K. V. and Surendran, P. K. (2006). Microbiological quality of farmed tropical freshwater prawn (*Macrobrachium rosenbergii*). *Journal of Aquatic Food Product Technology*, 15, 71 – 82.
- Leal, C., Codony, R., Compañó, R., Granados, M. and Prat, M.D. (2001). Determination of macrolide antibiotics by liquid chromatography, *Journal of Chromatography A*, 910, 285-290.
- Li, Y.X., Neufeld, K., Chastain, J., Curtis, A. and Velagaleti, P. (1998). Sensitive determination of erythromycin in human plasma by LC-MS/MS. *Journal of Pharmaceutical and Biomedical Analysis*, 16, 961-970.
- Masakazu, H., Rie, I., Terumitsu, Y., Yoji, H. and Hiroyuki, N. (1999). Determination of erythromycin and oleandomycin in meat and fish by LC/MS. *Journal of the Food Hygienic Society of Japan*, 40, 309-313.

- Norouzi, P., Daneshgar, P. and Ganjali, M.R. (2009). Electrochemical evaluation of non-electroactive drug Erythromycin in trace amount at biological samples by continuous cyclic voltammetry. *Materials Science and Engineering: C*, 29, 1281-1287.
- Schlüsener, M.P., Bester, K. and Spiteller, M. (2003). Determination of antibiotics such as macrolides, ionophores and tiamulin in liquid manure by HPLC-MS/MS. *Analytical and Bioanalytical Chemistry*, 375, 942-947.
- Tang, H.P., Ho, C. and Lai, S.S. (2006). High-throughput screening for multi-class veterinary drug residues in animal muscle using liquid chromatography/tandem mass spectrometry with on-line solid-phase extraction. *Rapid Communications in Mass Spectrometry*, 20, 2565 – 2572.
- Tran, T.T.H., Dang, T.H.O. and Nguyen, T.P. (2002). Study on diseases in giant freshwater prawns (*Macrobrachium rosenbergii*): A review.
- Wang, H.S., Zhang, A.M., Cui, H., Liu, D.J. and Liu, R.M. (2000). Adsorptive stripping voltammetric determination of erythromycin at a pretreated glassy carbon electrode. *Microchemical Journal*, 64, 67-71.
- Wang, J., Leung, D. and Lenz, S.P. (2006). Determination of five macrolide antibiotic residues in raw milk using liquid chromatography–electrospray ionization tandem mass spectrometry. *Journal of Agriculture and Food Chemistry*, 54, 2873–2880.
- Xiao, W., Chen, B., Yao, S. and Cheng, Z. (2005). Simultaneous determination of Erythromycin propionate and base in human plasma by high-performance liquid chromatography–electrospray mass spectrometry. *Journal of Chromatography B*, 817, 153–158.
- Zierfels, G. and Petz, M. (1994). Fluorimetric determination of Erythromycin residues in foods of animal origin after derivatization with FMOC and HPLC separation. *Z Lebensm Unters Forsch.*, 198, 307-312.